

## Information from Data File:

File :D:\RMP\12-501 ITEM 2.D

Operator : RMP

Acquired : 27 Mar 2012 12:58 using AcqMethod LOWBOIL.M

Sample Name: Proficiency Test

Misc Info : 12-501 ITEM 2

Vial Number: 4


Instrument : HP5975

Search Libraries: C:\Database\LIBA.L Minimum Quality: 90  
C:\Database\LIBT.L Minimum Quality: 80  
C:\Database\NIST08.L

Unknown Spectrum: Apex

Integration Params: rteint.p (RTEINT used)

Pk#	RT	Area%	Library/ID	Ref#	CAS#	Qual
1	2.41	100.00	C:\Database\NIST08.L Dimethyl sulfone	2507	000067-71-0	90

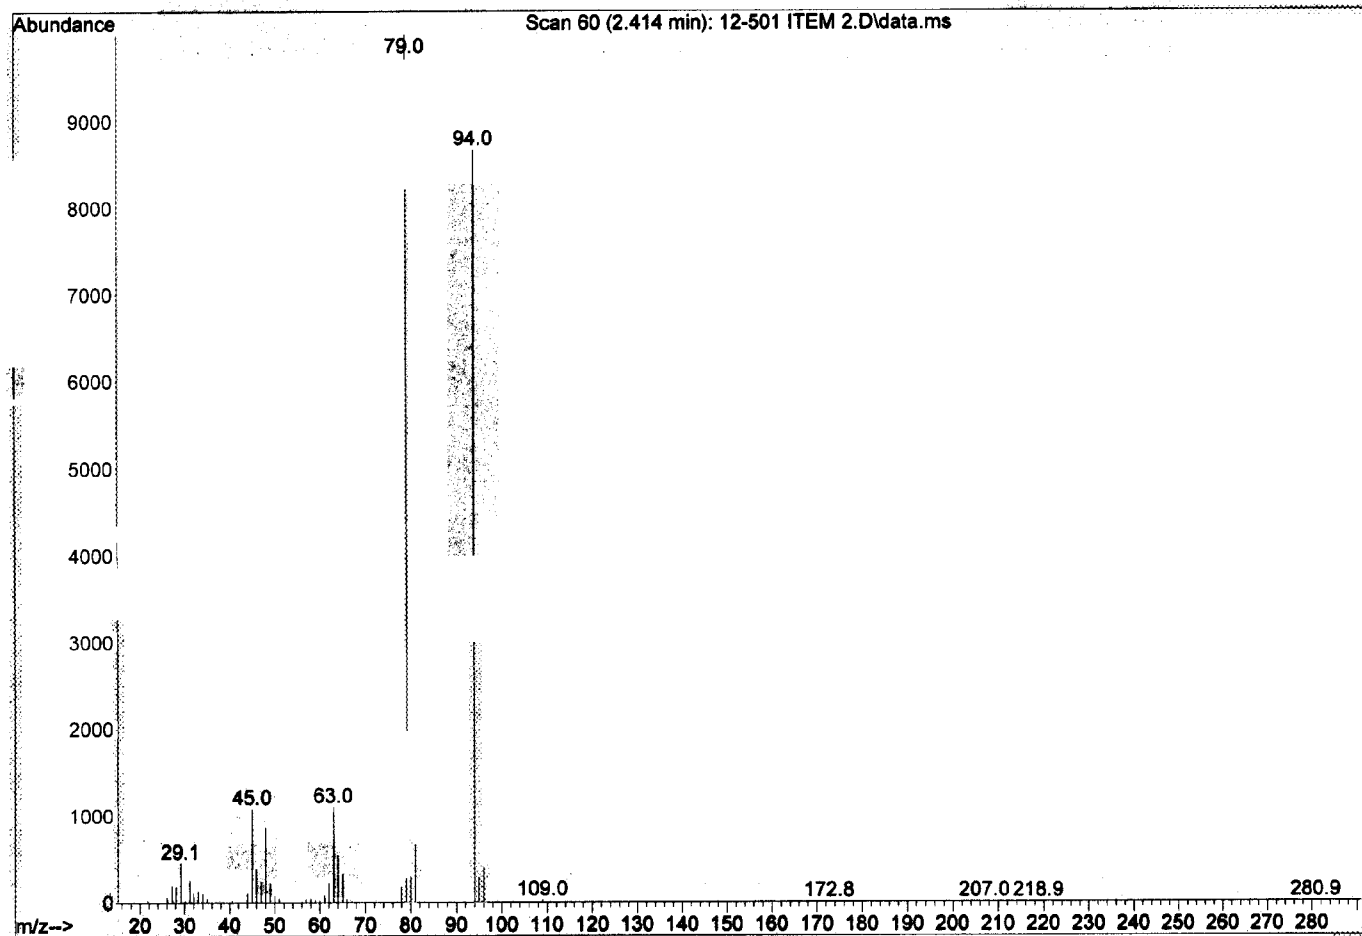

M/Z	Abundance	M/Z	Abundance	M/Z	Abundance
27.10	193	45.00	1081	65.00	326
28.10	185	46.00	390	78.00	182
29.10	455	47.00	241	79.00	10000
31.10	258	48.00	868	80.00	292
32.00	111	49.00	218	81.00	670
33.00	134	62.00	227	94.00	8670
34.00	102	63.00	1103	95.00	289
44.00	108	64.00	548	96.00	398